REED HEALTH & PERFORMANCE LLC

LOOK • FEEL • PERFORM

CERTIFICATE OF ANALYSIS

Quality You Can Trust.
Performance You Can Feel.

RHP-RT 20mg

Reed Health & Performance

This Certificate of Analysis verifies the identity, purity, and quality of RHP-RT. Each batch is third-party tested to ensure consistency, transparency, and the highest standards.

COA #: COA-2026-956205
Lot Number: RT20-0802
Labeled Content: 20mg
Volume: 3mL
Analysis Date: 06/10/2026
Date Received: 06/03/2026
Appearance: Good
Method: Full QC Panel

✓ PASS

PEPTIDE PURITY (HPLC)	NET PEPTIDE CONTENT	IDENTITY
99.94%	20.7 mg	Retatrutide
Spec: ≥ 95.0%	Report Only	Confirmed

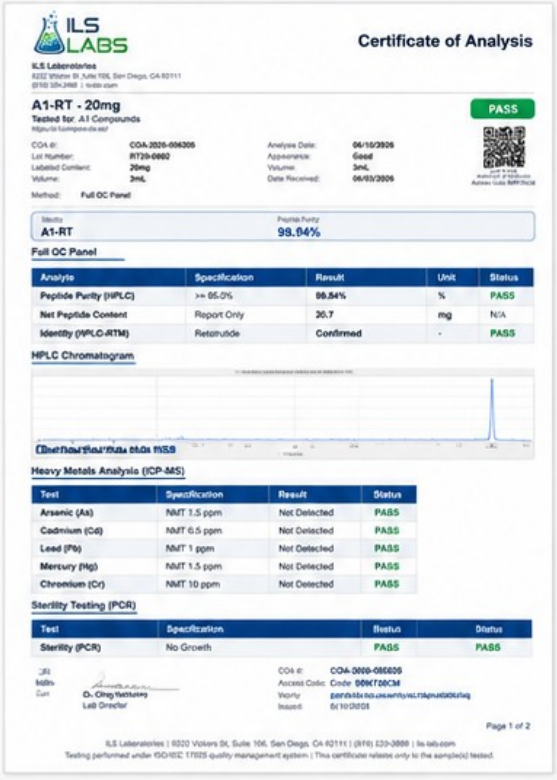
VIEW FULL COA REPORT

Verified by ILS Laboratories
Scan original COA for full details.

Third-Party Tested
Independently tested by ILS Laboratories.

Scan to View Original COA
Verify authenticity directly on the ILS Labs portal.

portal.ils-lab.com/verify
Access Code: 59M738CM


ILS LABS

Certificate of Analysis

ILS Laboratories

A1-RT - 20mg

Tested for: A1 Compounds

PASS

COA #:	COA-2026-956205	Analysis Date:	06/10/2026
Lot Number:	RT20-0802	Appearance:	Good
Labeled Content:	20mg	Volume:	3mL
Volume:	3mL	Date Received:	06/03/2026

Method: Full QC Panel

Identity	Peptide Purity
A1-RT	99.94%

Full QC Panel

Analyte	Specification	Result	Unit	Status
Peptide Purity (HPLC)	>= 95.0%	99.94%	%	PASS
Net Peptide Content	Report Only	20.7	mg	N/A
Identity (HPLC-RTM)	Retatrutide	Confirmed	-	PASS

HPLC Chromatogram

Heavy Metals Analysis (ICP-MS)

Test	Specification	Result	Status
Arsenic (As)	NMT 1.5 ppm	Not Detected	PASS
Cadmium (Cd)	NMT 0.5 ppm	Not Detected	PASS
Lead (Pb)	NMT 1 ppm	Not Detected	PASS
Mercury (Hg)	NMT 1.5 ppm	Not Detected	PASS
Chromium (Cr)	NMT 10 ppm	Not Detected	PASS

Sterility Testing (PCR)

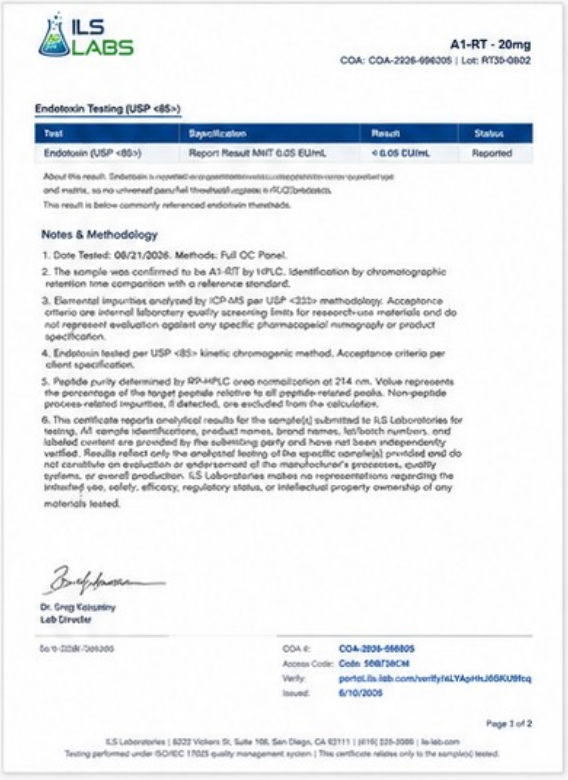
Test	Specification	Status	Status
Sterility (PCR)	No Growth	PASS	PASS

Dr. Greg Kaisamy
Lab Director

Page 1 of 2

ILS Laboratories | 8222 Vickers St, Suite 106, San Diego, CA 92111 | (619) 220-3080 | ils-lab.com

Testing performed under ISO/IEC 17025 quality management system | This certificate relates only to the sample(s) tested.


ILS LABS

A1-RT - 20mg

COA: COA-2026-956205 | Lot: RT20-0802

Endotoxin Testing (USP <85>)

Test	Specification	Result	Status
Endotoxin (USP <85>)	Report Result NMT 0.05 EU/mL	< 0.05 EU/mL	Reported

This result is below commonly referenced endotoxin thresholds.

Notes & Methodology

1. Date Tested: 06/21/2026. Methods: Full QC Panel.
2. The sample was confirmed to be A1-RT by HPLC. Identification by chromatographic retention time comparison with a reference standard.
3. Elemental impurities analyzed by ICP-MS per USP <232> methodology. Acceptance criteria are internal laboratory quality screening limits for research-use materials and do not represent evaluation against any specific pharmacopeial monograph or product specification.
4. Endotoxin tested per USP <85> kinetic chromogenic method. Acceptance criteria per client specification.
5. Peptide purity determined by RP-HPLC area normalization at 214 nm. Value represents the percentage of the target peptide relative to all peptide-related peaks. Non-peptide process-related impurities, if detected, are excluded from the calculation.
6. This certificate reports analytical results for the sample(s) submitted to ILS Laboratories for testing. All sample identifications, product names, brand names, lot/batch numbers, and labeled content are provided by the submitting party and have not been independently verified. Results reflect only the analyzed testing of the specific sample(s) provided and do not constitute an evaluation or endorsement of the manufacturer's processes, quality systems, or overall production. ILS Laboratories makes no representations regarding the intended use, safety, efficacy, regulatory status, or intellectual property ownership of any materials tested.

Dr. Greg Kaisamy
Lab Director

Page 2 of 2

ILS Laboratories | 8222 Vickers St, Suite 106, San Diego, CA 92111 | (619) 220-3080 | ils-lab.com

Testing performed under ISO/IEC 17025 quality management system | This certificate relates only to the sample(s) tested.

Every batch. Every time. Quality and transparency you can count on.

LOOK • FEEL • PERFORM